


Nano-Check™ Influenza+COVID-19 Dual Test


CLIA
WAIVED

FDA
CLEARED

- ✓ FDA 510(k) Cleared (k243561)
- ✓ FDA CLIA Waived (CW240029)
- ✓ Anterior Nasal Swab Specimen
- ✓ Evaluation conducted with an adequate number of positive samples
- ✓ Results in 15 minutes
- ✓ No Extra Steps
- ✓ Made in USA

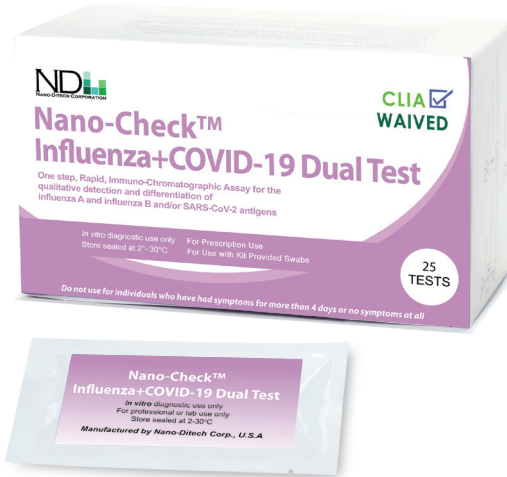

Easy/Simple To Use

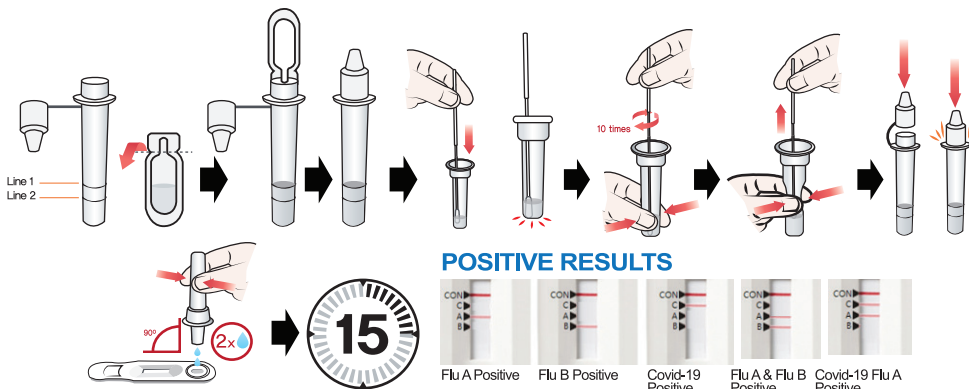

Contents

- Test Devices
- Ampules and Empty Reagent Tubes
- Sample collection swabs
- Positive control swab
- Negative control swab
- Instructions for Use
- Quick Reference Instruction

Performance Characteristics

SARS-CoV-2	Comparator RT-PCR		Total
	Positive	Negative	
Positive	232	3	235
Negative	33	1,701	1,734
Total	265	1,704	1,969

Flu A	Comparator RT-PCR		Total
	Positive	Negative	
Positive	417	6	423
Negative	63	1,483	1,546
Total	480	1,489	1,969

Flu B	Comparator RT-PCR		Total
	Positive	Negative	
Positive	99	5	104
Negative	15	1,850	1,865
Total	114	1,855	1,969

Positive Percent Agreement = 87.6%
Negative Percent Agreement = 99.8%

Positive Percent Agreement = 86.9%
Negative Percent Agreement = 99.6%

Positive Percent Agreement = 86.8%
Negative Percent Agreement = 99.7%

Refer to IFU for additional LOD/Analytical Reactivity/Clinical Performance Information

Ordering Information

Cat. No.: MD8154 (25 Tests)

ND
NANO-DITECH CORPORATION

AQUEOUS
DIAGNOSTICS

For a quote and orders: orders@aqueousdx.com

[AqueousDx.com](https://www.aqueousdx.com)